


SUPPLEMENTARY TABLE

Supplementary Table 1: Pentacam parameters before and after treatment of the ocular surface.

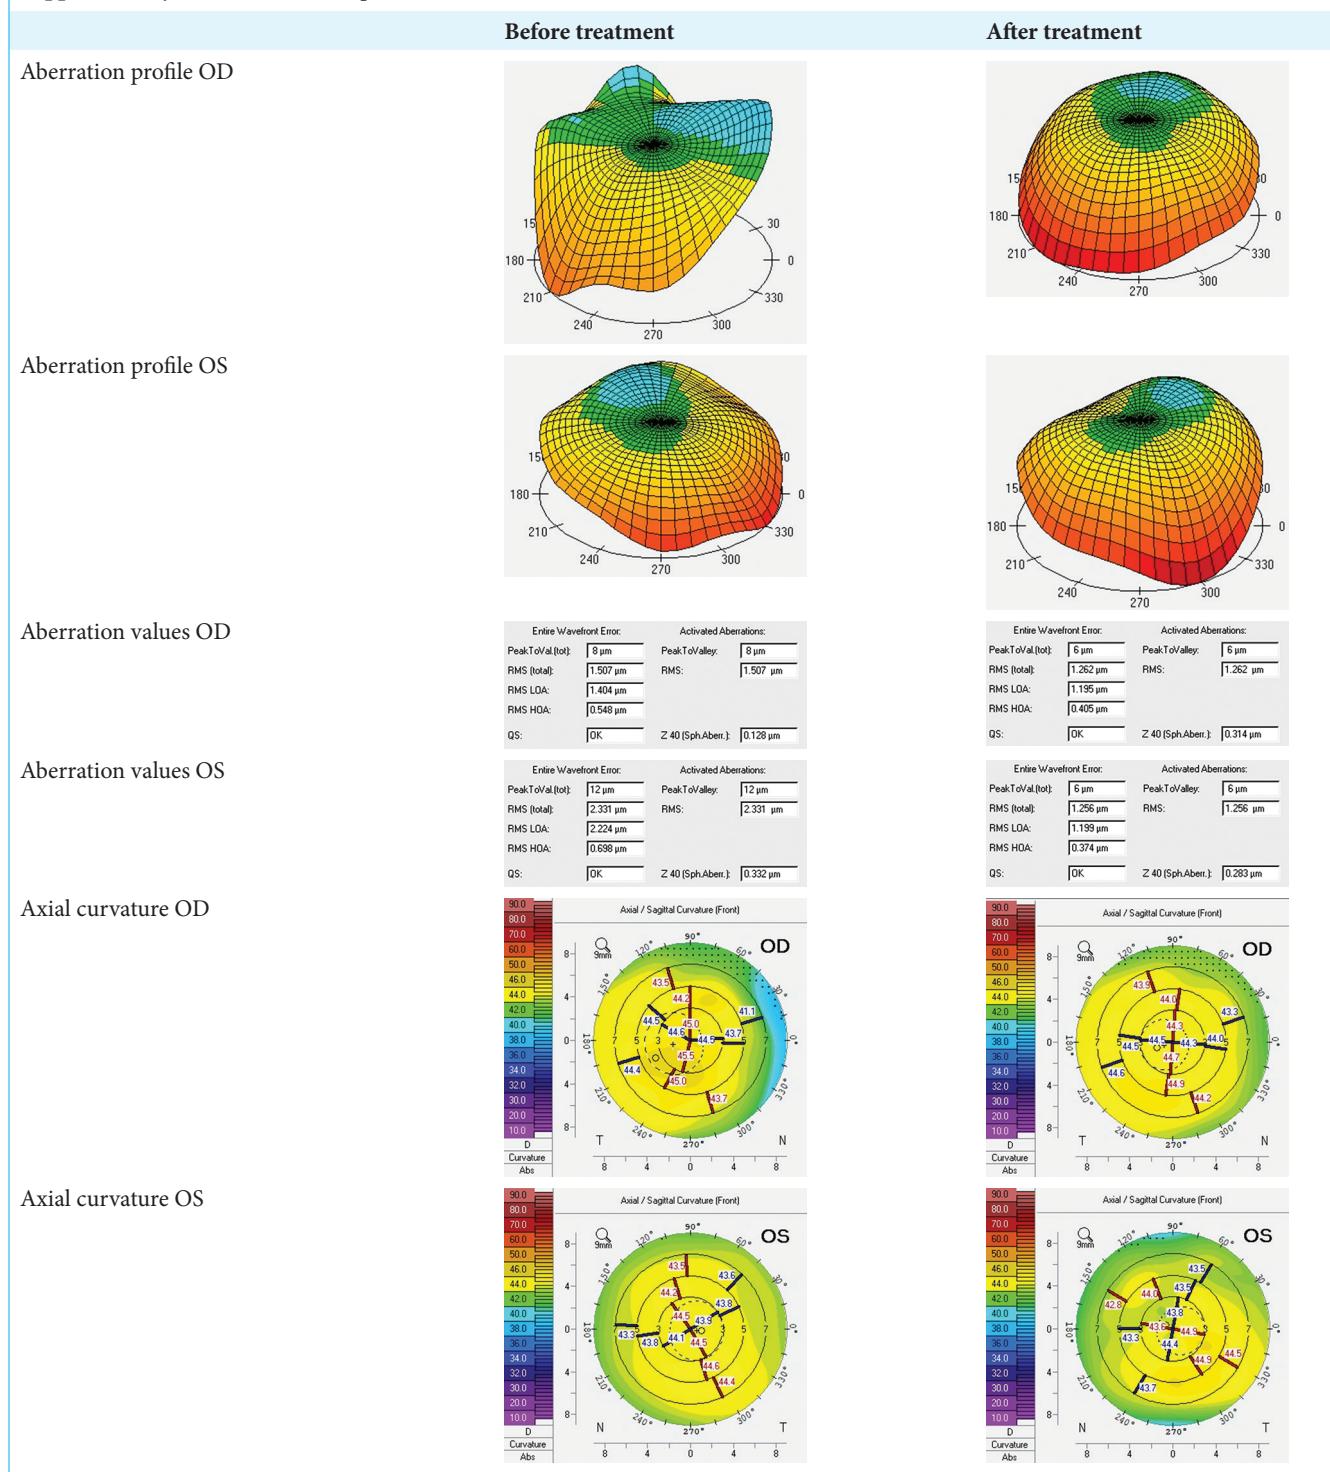

(Contd...)